



## PRODUCT SPECIFICATION SHEET

### Buffered Glucose Broth / Glucose Phosphate Broth (MR-VP Medium) (DM142)

#### Intended use

MR-VP Medium (Glucose Phosphate Broth/Buffered Glucose Broth) (DM142) is used for performing the Methyl Red and Voges Proskauer tests in differentiation of coli-aerogenes group.

#### Product Summary and Explanation

This glucose-phosphate medium is recommended for the Methyl-red and Voges-Proskauer tests, for the differentiation of the coli-aerogenes group<sup>(1)</sup>. In 1915, Clark and Lubs<sup>(2)</sup> demonstrated that the colon-aerogenes family of bacteria could be divided into two groups based on their action in a peptone and dextrose medium. When tested with pH indicator Methyl red, the "coli" group produced high acidity while the "aerogenes" group produced a less acid reaction. The test to detect high acid end product is known as the Methyl Red (MR) test. This test distinguishes those organisms able to form large amounts of acid from glucose so that the pH falls below 4.4 produce low pH level. Voges and Proskauer<sup>(3)</sup> described a red fluorescent coloration which appeared after the addition of potassium hydroxide to cultures of certain organisms in glucose medium. The coloration was shown to be due to the oxidation of the acetylmethyl-carbinol producing diacetyl which reacts with the peptone of the medium to give a red color<sup>(4,5)</sup>. This is known as (VP) test. The MR and VP test appear in the identification of scheme for the Enterobacteriaceae<sup>(6)</sup> which are important isolates in clinical microbiology, as well as in the microbiology of foods and dairy products.

#### Principles of the Procedure

All members of the Enterobacteriaceae convert glucose to pyruvate by the Embden-Meyerhof pathway. Some bacteria metabolize pyruvate by the mixed acid pathway and produce acidic end products (pH < 4.4), such as lactic, acetic and formic acids. Other bacteria metabolize pyruvate by the butylenes glycol pathway and produce neutral end products (pH > 6.0), one of which is acetoin (acetylmethylcarbinol). In the MR test, the pH indicator methyl red detects acidic end products<sup>(7)</sup>. In the VP test, acetoin is oxidized in the presence of oxygen and potassium hydroxide (KOH) to diacetyl, which produces a red color.<sup>(8)</sup>

#### Formula / Liter

Ingredients	Gms / Litre
Buffered peptone	7.00
Dextrose	5.00
Dipotassium hydrogen phosphate	5.00
Final pH: 6.9 ± 0.2 at 25°C	
Formula may be adjusted and/or supplemented as required to meet performance specifications	

#### Precautions

1. For Laboratory Use only.
2. IRRITANT. Irritating to eyes, respiratory system, and skin.

#### Directions

1. Suspend 17 grams in 1000 ml of distilled water.
2. Heat if necessary to dissolve the medium completely.
3. Distribute in test tubes in 10 ml amounts.
4. Sterilize by autoclaving at 15 lbs pressure (121°C) for 15 minutes





## PRODUCT SPECIFICATION SHEET



### Quality Control Specifications

Dehydrated Appearance	Cream to yellow colored, homogeneous, free flowing powder
Prepared Medium	Light yellow coloured clear solution without any precipitate
Reaction of 1.7% Solution	pH : 6.9 ± 0.2
Gel Strength	Not Applicable

**Expected Cultural Response:** Cultural characteristics observed after an incubation at 30-32°C for 18-48 hours.

Sr. No.	Organisms	Results to be achieved			
		Inoculum (CFU)	Growth	MR Test	VP Test
1.	<i>Escherichia coli</i> ATCC 25922	50 -100	Luxuriant	Positive reaction, bright red colour	Negative reaction
2.	<i>Enterobacter aerogenes</i> ATCC 13048	50 -100	Luxuriant	Negative reaction	Positive reaction, eosin pink/red colour within 2-5 minutes
3.	<i>Klebsiella pneumoniae</i> ATCC 23357	50-100	Luxuriant	Negative reaction	Positive reaction, eosin pink / red colour within 2-5 minutes

The organisms listed are the minimum that should be used for quality control testing.

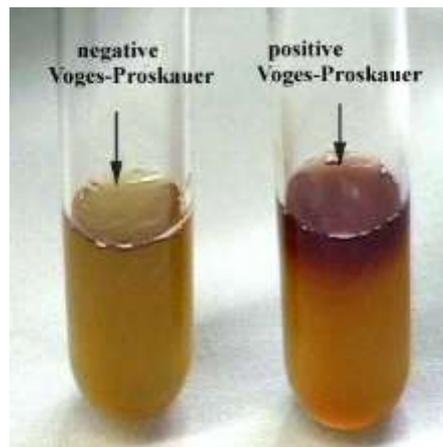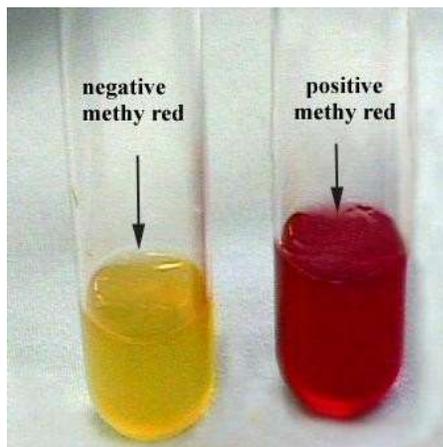

### Test Procedure

1. Inoculate MR-VP Medium with growth from single colony.
2. Incubate at 35± 2°C for 48 hours.
3. Test as follows

#### Methyl Red Test

1. Transfer 2.5 ml of the MR-VP Medium culture to a tube (13x100mm).
2. Add 5 drops of methyl red indicator and observe for a colour change.

#### VP Test

1. Transfer 2.5 ml of the MR-VP Medium culture to a tube (13x100mm).
2. Add 0.3 ml (6 drops) of Voges-Proskauer Reagent A (5% α-naphthol).
3. Add 0.1 ml (2 drops) of Voges-Proskauer Reagent B (40% KOH).
4. Gently agitate the tube and let stand for 10 to 15 minutes.
5. Observe for color change.





## PRODUCT SPECIFICATION SHEET

---

### Results

#### Methyl Red (MR) Test

Positive: Bright red color.

Negative: Yellow-orange color.

Note: If the test is negative, continue to incubate the broth without added reagent; repeat test after an additional 18 to 24 hours incubation.

#### Voges-Proskauer (VP) Test

Positive: Red color.

Negative: No red color.

### Storage

Store the sealed bottle containing the dehydrated medium at 10 - 30°C. Once opened and recapped, place container in a low humidity environment at the same storage temperature. Protect from moisture and light.

### Expiration

Refer to the expiration date stamped on the container. The dehydrated medium should be discarded if not free flowing, or if the appearance has changed from the original color. Expiry applies to medium in its intact container when stored as directed.

### Limitations of the Procedure

1. The MR-VP reactions are only part of the tests required to identify organisms.
2. Each laboratory should standardize on the inoculum density, volume of broth and the test container size.
3. MR test requires a minimum incubation of 48 hours before the pH indicator is added.
4. When using Barritt's reagent add  $\alpha$ -naphthol first and KOH second; do not reverse this order.
5. Vaughn et al. (7) warned of false positive VP reactions if the completed tests are left standing for over an hour.

### Packaging

**Product Name :** MR-VP Medium (Glucose Phosphate Broth) Product

**Code :** DM142

**Available Pack sizes :** 100gm / 500gm

### References

1. DHSS Report 71 (1982), The bacteriological Examination of Drinking Water Supplies, HMSO London.
2. Clark, W.M., and H.A. Lubs. 1915. The differentiation of bacteria of the colon-aerogenes family by the use of indicators. J. infect. Dis. 17:160-173.
3. Voges O. and Proskauer B. (1898) Z. f. Hyg. 28:20-22.
4. Harden A. and Walpole G.S. (1906) Proc. Roy. Soc. B. 77:399
5. Harden A. and Norris D. (1911) Physiol. 42:332.
6. Farmer, J.J., III. 1995. Enterobacteriaceae: Introduction and identification, p.438-499. In P.R. Murray, E.J. Baron, M.A. Tenover, and F.C. Tenover, and R.H. Tenover (ed), Manual of clinical microbiology, 6<sup>th</sup> ed. American Society for Microbiology, Washington, D.C.
7. Vaughn R., Mitchell N. B. and Levine M. (1939) J. Amer. Water Works Assn. 31:993-1000 DHSS Report

### Further Information

For further information please contact your local MICROMASTER Representative.





## PRODUCT SPECIFICATION SHEET

---



**MICROMASTER LABORATORIES PRIVATE LIMITED**

Unit 38/39, Kalpataru Industrial Estate,  
Off G.B. Road, Near 'R-Mall', Thane (W) - 400607. M.S. INDIA.  
Ph: +91-9320126789/9833630009/9819991103  
Email: [sales@micromasterlab.com](mailto:sales@micromasterlab.com)

DM142PSS,QAD/FR/024,Rev.00

**Disclaimer :**

All Products conform exclusively to the information contained in this and other related Micromaster Publications. Users must ensure that the product(s) is appropriate for their application, prior to use. The information published in this publication is based on research and development work carried out in our laboratory and is to the best of our knowledge true and accurate. Micromaster Laboratories Pvt Ltd reserves the right to make changes to specifications and information related to the products at any time. Products are intended for laboratory, diagnostic, research or further manufacturing use only and not for human or animal or therapeutic use, unless otherwise specified. Statements included herein should not be considered as a warranty of any kind, expressed or implied, and no liability is accepted for infringement of any patent.

